

MAY 28 2002

page 1 of 9

**TSRH® Spinal System
510(k) Summary
February 2002**

- I. Company:** Medtronic Sofamor Danek USA, Inc.
1800 Pyramid Place
Memphis, TN 38132
(901) 396-3133
- II. Proposed Proprietary Trade Name:** TSRH® Spinal System
- III. Description**

The purpose of this 510(k) submission is to add the indication of degenerative disc disease to the TSRH® Spinal System.

The TSRH® Spinal System is intended to help provide immobilization and stabilization of spinal segments as an adjunct to fusion of the thoracic, lumbar, and/or sacral spine.

The TSRH® Spinal System consists of a variety of shapes and sizes of rods, hooks, screws, cross connectors, and connecting components. In addition, GDLH® rods, DYNALOK PLUS™ bolts, CD HORIZON® Low Profile MULTI-SPAN® CROSSLINK® Plates, GDLH® rod/bolt connectors, GDLH® Variable Angle T-Bolts, and GDLH® and CD HORIZON® set screws and locking screws may be used with the TSRH® Spinal System.

The TSRH® Spinal System implant components can be rigidly locked into a variety of configurations, with each construct being tailor-made for the individual case. The hooks are intended for posterior use only and the staples are for anterior use only. The TSRH-3D™ connectors and TSRH-3D™ screws are intended for posterior use only. All CROSSLINK® Plates are for posterior use and the CROSSLINK Axial and Offset Plates may be used anteriorly as well.

The TSRH Spinal System components are fabricated from stainless steel conforming to ASTM F-138 or ISO 5832-1 or ISO 5832-9. Alternatively, they may be fabricated from medical grade titanium alloy conforming to ASTM F-136 or ISO 5832-3 or medical grade titanium conforming to ASTM F67. The TSRH Spinal System may be sold sterile or non-sterile.

IV. Indications for Use:

When used as a pedicle screw fixation system of the non-cervical posterior spine in skeletally mature patients, the TSRH® Spinal System is indicated for one or more of the following: (1) degenerative disc disease (defined as back pain of discogenic origin with degeneration of the disc confirmed by patient history and radiographic studies), (2) degenerative spondylolisthesis with objective evidence of neurologic impairment, (3) fracture, (4) dislocation, (5) scoliosis, (6) kyphosis, (7) spinal tumor, and/or (8) failed previous fusion (pseudarthrosis).

In addition, when used as a pedicle screw fixation system, the TSRH® Spinal System is indicated for skeletally mature patients: (1) having severe spondylolisthesis (Grades 3 and 4) of the fifth lumbar-first sacral (L5-S1) vertebral joint; (2) who are receiving fusions using autogenous bone graft only; (3) who are having the device fixed or attached to the lumbar and sacral spine (L3 and below); and (4) who are having the device removed after the development of a solid fusion mass.

When used as a posterior, non-cervical, non-pedicle screw fixation system, the TSRH® Spinal System is intended for the following indications: (1) degenerative disc disease (as defined by back pain of discogenic origin with degeneration of the disc confirmed by patient history and radiographic studies), (2) spondylolisthesis, (3) fracture, (4) spinal deformities (i.e., scoliosis, kyphosis, and/or lordosis), (5) spinal stenosis, (6) pseudarthrosis, (7) tumor resection, and/or (8) unsuccessful previous attempts at spinal fusion.

For anterior use only the TSRH® Spinal System has the additional indications of: (1) spinal stenosis and/or, (2) spondylolysis.

- V. The TSRH® Spinal System was declared substantially equivalent to the TOWNLEY Pedicle Screw Plating System and the CD® Spinal System manufactured by Medtronic Sofamor Danek along with other systems, for the pedicle screw indication of degenerative disc disease. Mechanical test data were provided in this application.



DEPARTMENT OF HEALTH & HUMAN SERVICES

Public Health Service

Food and Drug Administration
9200 Corporate Boulevard
Rockville MD 20850

MAY 28 2002

Richard W. Treharne, Ph.D.
Senior Vice President, Regulatory Affairs
Medtronic Sofamor Danek
1800 Pyramid Place
Memphis, Tennessee 38132

Re: K020699

Trade/Device Name: TSRH® Spinal System

Regulation Number: 21 CFR 888.3060 and 888.3070

Regulation Name: Spinal intervertebral body fixation orthosis and Pedicle screw spinal system

Regulatory Class: II

Product Code: KWP, MNH, MNI, KWQ

Dated: February 25, 2002

Received: March 1, 2002

Dear Dr. Treharne:

We have reviewed your Section 510(k) premarket notification of intent to market the device referenced above and have determined the device is substantially equivalent (for the indications for use stated in the enclosure) to legally marketed predicate devices marketed in interstate commerce prior to May 28, 1976, the enactment date of the Medical Device Amendments, or to devices that have been reclassified in accordance with the provisions of the Federal Food, Drug, and Cosmetic Act (Act) that do not require approval of a premarket approval application (PMA). You may, therefore, market the device, subject to the general controls provisions of the Act. The general controls provisions of the Act include requirements for annual registration, listing of devices, good manufacturing practice, labeling, and prohibitions against misbranding and adulteration.

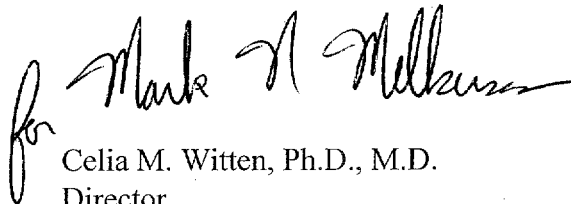
If your device is classified (see above) into either class II (Special Controls) or class III (PMA), it may be subject to such additional controls. Existing major regulations affecting your device can be found in the Code of Federal Regulations, Title 21, Parts 800 to 898. In addition, FDA may publish further announcements concerning your device in the Federal Register.

Please be advised that FDA's issuance of a substantial equivalence determination does not mean that FDA has made a determination that your device complies with other requirements of the Act or any Federal statutes and regulations administered by other Federal agencies. You must comply with all the Act's requirements, including, but not limited to: registration and listing (21 CFR Part 807); labeling (21 CFR Part 801); good manufacturing practice requirements as set forth in the quality systems (QS) regulation (21 CFR Part 820); and if applicable, the electronic product radiation control provisions (Sections 531-542 of the Act); 21 CFR 1000-1050.

This letter will allow you to begin marketing your device as described in your Section 510(k) premarket notification. The FDA finding of substantial equivalence of your device to a legally marketed predicate device results in a classification for your device and thus, permits your device to proceed to the market.

If you desire specific advice for your device on our labeling regulation (21 CFR Part 801 and additionally 21 CFR Part 809.10 for in vitro diagnostic devices), please contact the Office of Compliance at (301) 594-4659. Additionally, for questions on the promotion and advertising of your device, please contact the Office of Compliance at (301) 594-4639. Also, please note the regulation entitled, "Misbranding by reference to premarket notification" (21CFR Part 807.97). Other general information on your responsibilities under the Act may be obtained from the Division of Small Manufacturers, International and Consumer Assistance at its toll-free number (800) 638-2041 or (301) 443-6597 or at its Internet address <http://www.fda.gov/cdrh/dsma/dsmamain.html>

Sincerely yours,

for Mark H. Melanson

Celia M. Witten, Ph.D., M.D.
Director
Division of General, Restorative
and Neurological Devices
Office of Device Evaluation
Center for Devices and
Radiological Health

Enclosure

510(k) Number (if known): K020699Device Name: TSRH® Spinal System**Indications for Use:**

When used as a pedicle screw fixation system of the non-cervical posterior spine in skeletally mature patients, the TSRH® Spinal System is indicated for one or more of the following: (1) degenerative disc disease (defined as back pain of discogenic origin with degeneration of the disc confirmed by patient history and radiographic studies), (2) degenerative spondylolisthesis with objective evidence of neurologic impairment, (3) fracture, (4) dislocation, (5) scoliosis, (6) kyphosis, (7) spinal tumor, and/or (8) failed previous fusion (pseudarthrosis).

In addition, when used as a pedicle screw fixation system, the TSRH® Spinal System is indicated for skeletally mature patients: (1) having severe spondylolisthesis (Grades 3 and 4) of the fifth lumbar-first sacral (L5-S1) vertebral joint; (2) who are receiving fusions using autogenous bone graft only; (3) who are having the device fixed or attached to the lumbar and sacral spine (L3 and below); and (4) who are having the device removed after the development of a solid fusion mass.

When used as a posterior, non-cervical, non-pedicle screw fixation system, the TSRH® Spinal System is intended for the following indications: (1) degenerative disc disease (as defined by back pain of discogenic origin with degeneration of the disc confirmed by patient history and radiographic studies), (2) spondylolisthesis, (3) fracture, (4) spinal deformities (i.e., scoliosis, kyphosis, and/or lordosis), (5) spinal stenosis, (6) pseudarthrosis, (7) tumor resection, and/or (8) unsuccessful previous attempts at spinal fusion.

For anterior use only the TSRH® Spinal System has the additional indications of: (1) spinal stenosis and/or, (2) spondylolysis.

(PLEASE DO NOT WRITE BELOW THIS LINE—CONTINUE ON ANOTHER PAGE IF NEEDED)

Concurrence of CDRH, Office of Evaluation (ODE)

Prescription Use _____
(Per 21 CFR 801.109)
(Optional 1-2-96)

OR

Over-the-counter Use _____

for Mark N. Milken
(Division Sign-Off)
Division of General, Restorative
and Neurological Devices

510(k) Number K020699

380008